


Taric® Anesthesia Workstations





Health care has become an increasingly complex field. Providing state-of-the-art care at every step It needs modern technology, and doing so is often possible but needs to choose the right tools and at a reasonable cost to achieve impressive results.

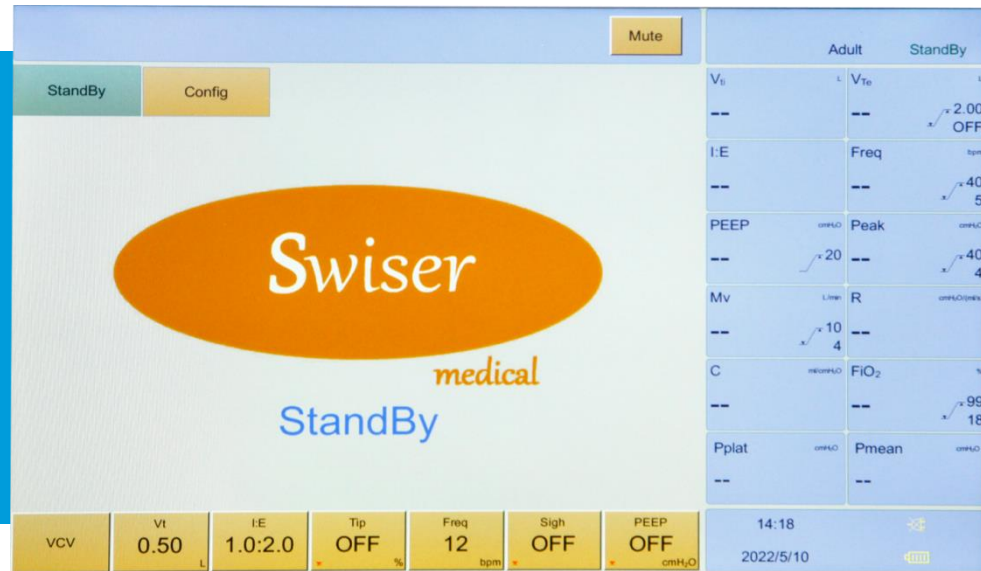

It combines modern design with the latest technology to meet the demand for an innovative and comprehensive anesthesia solution for today's increasingly complex medical environments. Innovative design provides workflow support during OT.






Step up to the high standard of anesthesia workstations and experience new levels of performance, efficiency and safety.



Technique Specifications	
Physical Specifications	
Dimensions:	70*85*140cm
Weight:	65kg
Casters:	Front wheels with lock
Screen:	12.1 inch LCD
Working Specifications	
Power	AC 220V±10%, 50Hz±2%
Pipeline Supply	
Gas configuration	O ₂ , N ₂ O, Air
Pipeline input range	280-600kPa
Battery Power	
Run-time	≥180 mins
Pre-setting Functions	
Language	English
Calibration	Automatic
Applications	
Patient range	Audlt/ Pediatric
Ventilator Specifications	
Modes of Ventilation	
VCV	Volume Controlled Ventilation
SIMV-V	Synchronized Intermittent Mandatory Ventilation-Volume
SIMV-P	Synchronized Intermittent Mandatory Ventilation-Pressure
MANUAL	Manual
A/C	Assist / control Ventilation
PCV	Pressure Control Ventilation
PSV	Pressure Support Ventilation
STAND-BY	STAND-BY
Ventilator Parameter	
Working type	Electronic control, pneumatic driven
Tidal Volume range	20-1500ml
Pressure range	5-60 cmH ₂ O
Rispiration rate range	1-100 bpm (1-40bpm under SIMV)
I:E range	4:1-1:8
Ptrigger range	-20-20 cmH ₂ O (based on PEEP)
Flow trigger	0-15L
Minute volume range	>18L/Min
SIGH range	0-5/100

System Standard	
Hypoxic guard system	N ₂ O cut-off valve, O ₂ concentration >25%
Safety valve	<12.5kPa
Fresh gas compensation	25-75L/min
Volume of CO ₂ absorber	2 L
Flow meter	5 tubes, Cascade 0.1-15L/min O ₂ 0.1-15L/min N ₂ O, 0.1-15L/min air
Vaporizer	2 Selectetac, maximum 2 mounts(Isoflurane/Enflurane/Sevoflurane/Halothane)
Monitoring	
Display graphics	Waveforms of P-T, F-T, V-T, loops of P-V,V-F,F-P(Zoom in/out, comparison, freeze)
Types	VT, MV, BPM, Paw, Lung compliance, Inspiratory Platform,FiO ₂
Alarm Limits	
Audio/Visual	No tidal volume, MV,Paw, FiO ₂ limitation O ₂ , Air failure, AC power failure, Battery low
PEEP	
Type	Integrated, Electronic control
Range	OFF, 3-30cmH ₂ O
Optional	
1.AGSS	Anesthetic Gas Scavenging Systems
2.Suction Unit	
3.Communication Interface	Ethernet, USB, VGA
4.Auxiliary Oxygen meter	

CORPORATE HEADQUARTERS

Swiser medical Ltd
6 prospect street HD12NX
Huddersfeild, England
+44 7463 014493 
www.swisermed.com